

Standard Test Method for Determination of Residual Acetaldehyde in Polyethylene Terephthalate Bottle Polymer Using an Automated Static Head-Space Sampling Device and a Capillary GC with a Flame Ionization Detector¹

This standard is issued under the fixed designation F 2013; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ε) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers a gas chromatographic procedure for the determination of the ppm residual acetaldehyde (AA) present in poly(ethylene terephthalate) (PET) homopolymers and co-polymers which are used in the manufacture of beverage bottles. This includes sample types of both amorphous and solid-stated pellet and preform samples, as opposed to the bottle test, Test Method D 4509, an acetaldehyde test requiring 24 h of desorption time at 23°C into the bottle headspace and then the concentration of the headspace quantified by a similar GC method.

1.2 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:²

D 4509 Test Methods for Determining the 24-Hour Gas (AIR) Space Acetaldehyde Content of Freshly Blown PET Bottles³

E 691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method

3. Terminology

3.1 The terms employed in this test method are commonly used in normal laboratory practice and require no special comment.

¹ This test method is under the jurisdiction of ASTM Committee F02 on Flexible Barrier Materials and is the direct responsibility of Subcommittee F02.15 on Chemical/Safety Properties.

Current edition approved April 1, 2005. Published September 2005. Originally approved in 2000 as published as F 2013–00. Last previous edition approved in 2001 as F 2013–01.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ Withdrawn.

4. Summary of Test Method

4.1 A specified size (800 to 1000 µm) of granulated sample is weighed into a 20-mL head-space vial, sealed, and then heated at 150°C for 60 min. After heating, the gas above the sealed sample of PET polymer is injected onto a capillary GC column. The acetaldehyde is separated, and the ppm of acetaldehyde is calculated.

5. Significance and Use

5.1 This test method is of particular use as a quality control tool for a molding or synthesis operation. Acetaldehyde is a volatile degradation product generated during melt processing of PET. Thus, it becomes trapped in the sidewalls of a molded article and desorbs slowly into the contents packaged therein. In some foods and beverages AA can impart an off-taste that is undesirable, thus, it is important to know its concentration in PET articles that are to be used in food contact applications.

5.2 The desorption conditions of 150 C for 60 min are such that no measurable AA is generated by the sample during the desorption process.

6. Sources of Error

6.1 A bias is known to exist if the ratio of sample mass (mg) to head-space vial volume (mL) exceeds a value of ten.

6.2 Acetaldehyde is very volatile and must be handled carefully to avoid sample loss during the calibration procedure. Storing the standard vials in a refrigerator is a must to minimize the error due to volatility.

6.3 Failure to achieve a tight seal on the head-space vial will result in the loss of acetaldehyde during storage and desorption, producing a false low value.

6.4 Failure to grind the sample to the appropriate particle size may lead to a false low value for residual AA due to the increased path length for desorption.

6.5 Samples submitted for "residual AA measurement" should be stored in a freezer until they are tested. Failure to do so can result in lower than expected results.

6.6 Excessive grinding of samples can cause residual AA contained therein to be desorbed. Extensive excessive grinding can lead to actual melting of the polymer and AA generation. Samples which have been chilled in liquid nitrogen properly should only be in the grinder for ~30 s or less.

7. Apparatus

7.1 *Gas Chromatograph.*

7.2 *Integrator.*

7.3 *Head-Space Sampler.*

7.4 *Column*, 30-m by 0.53-mm inside diameter (megabore capillary column).

7.5 *Vials*, 20-mL, head-space, with 20-mm septa, 20-mm aluminum caps, and crimper for 20-mm caps.

7.6 *Crimper*, 20-mm.

7.7 *Decrimper*, 20-mm.

7.8 *Wiley Mill*, equipped with an 800 to 1000- μm screen, or equivalent.

7.9 *Syringe*, calibrated, with certificate of calibration.

7.10 *Small Vacuum Cleaner*, with hose attachment for cleaning.

7.11 *Analytical Balance*, capable of accurately weighing to at least ± 0.0001 g.

7.12 *Hammer.*

8. Reagents and Materials

8.1 *Acetaldehyde (AA)*, 500 ppm AA in water (or 1000 ppm), purchased certified standard.

8.2 *Liquid Nitrogen*, plant grade (R-3, S-3).

9. Calibration and Standardization

NOTE 1—The following procedure should be performed and recorded once every three months.

9.1 Break open a certified AA standard ampule (ampules must be stored in a refrigerator) or prepare AA standard by the attached supplemental procedure. (See [Appendix X5](#).)

9.2 Using the syringe, fill it by placing the tip in the liquid standard and quickly moving the plunger up and down several time to evacuate any bubbles, then pull the plunger back past the 2.000- μL mark to 2.200 to 2.250 μL .

9.3 Wipe the syringe needle with a tissue.

9.4 Depress the plunger until the digital readout is 2.000 μL .

9.5 Smear the excess liquid that is on the syringe tip on the OUTSIDE of the headspace vial.

9.6 Place the syringe inside of the vial so that the tip just touches the bottom of the vial.

9.7 Quickly inject the liquid standard into the vial and swirl the syringe tip around the inside of the vial to smear all liquid on the vial walls.

9.8 Remove the syringe and IMMEDIATELY cap the vial.

9.9 Calculate the weight of AA based on the standard's certified value and a 2.000- μL injection volume.

NOTE 2—Acetaldehyde is very volatile. The AA ampules must be stored in a refrigerator, and the standards prepared immediately after breaking open an ampule.

9.10 Analyze the working standard by the procedure described in Section 11, starting with [11.2.11](#).

9.11 Calculate an AA response factor for the standard using the following equation:

$$\text{response factor of AA} = \text{Wt of AA in } \mu\text{g}/\text{area of AA} \quad (1)$$

NOTE 3—Due to the error associated with the certified standard, [9.1-9.11](#) should be performed five times using five different standard ampules.

9.12 Average the five response factors obtained, and use this value for the sample analyses.

9.13 Manually enter the calculated response factor in the calibration list of the integrator or data system.

NOTE 4—During a series of sample analyses, a periodic check of instrument performance is recommended by placing a few liquid standard samples throughout the sample set. If these values fall out of the acceptable range as specified by the certificate of analysis, recalibration ([9.1-9.12](#)) should be performed.

10. Sample Preparation

10.1 *Parisons or Preforms or Plaques*—May be cryogenically ground whole, or can be broken into small pieces with a hammer (using liquid nitrogen) and then ground with the aid of grinding mill equipped with a 20-mesh or 850- μm screen. The grind should be thoroughly homogenized before sampling for AA. If the appropriate size screen is not available on the large grinding mill, then it is suggested that the sample be ground to 3 to 6 mm on the large mill and the sample thoroughly homogenized. A portion can then be taken to a smaller mill equipped with the 20-mesh or 850- μm screen and cryogenically ground again before analysis. Again the final sample should be thoroughly homogenized.

10.2 *Pellets*—May be cryogenically ground in a small grinding mill using liquid nitrogen. The final sample should be thoroughly homogenized before sampling for analysis.

NOTE 5—Samples, either preforms, plaques, or pellets, should be chilled in the liquid nitrogen for several minutes until the liquid nitrogen stops boiling and then dropped immediately into the grinder. Sample should be sufficiently ground in a few seconds. The grinder should not be allowed to operate more than 20 to 30 s as in such cases undesirable sample heating can occur.

11. Procedure

NOTE 6—Refer to the general operating manual for gas chromatograph, the head-space sampler, and the series integrator for instructions in performing steps in this procedure.

11.1 Adjust the gas chromatograph to the conditions specified in [Appendix X1](#). Adjust the head-space sampler to the conditions in [Appendix X2](#). Set the series integrator to the conditions in [Appendix X3](#).

11.2 *Sample Analysis:*

11.2.1 Place 2 to 3 of polymer pellets (or crushed preform) into a small Dewar flask.

11.2.2 Cover the polymer with 20 to 40 mL of liquid nitrogen.

11.2.3 Allow the polymer to chill under the liquid nitrogen for approximately 3 min (or until most of the liquid N₂ has evaporated).

11.2.4 Turn on the Wiley mill equipped with a 800 to 1000- μm screen.

11.2.5 Slowly pour the remaining liquid nitrogen from the Dewar flask through the Wiley mill, followed by the chilled polymer sample (tapping the sample may be required).

11.2.6 Collect the ground polymer in a small glass jar or small manila envelope.

11.2.7 Turn off the Wiley mill and clean it with a vacuum cleaner.

11.2.8 Allow the ground polymer sample to come to room temperature (approximately 10 min).

11.2.9 Weigh approximately 0.2000 (± 0.0200) g, recorded to the nearest 0.0001 g, into a 20-mL head-space vial.

11.2.10 Place a septum (with TFE-fluorocarbon side down towards the inside of the vial) on the vial. Place an aluminum cap on top of the septum, and crimp the cap with a crimper UNTIL THE CAP CANNOT BE TURNED. Remove the center piece of the aluminum cap (if it exists).

11.2.11 Place the vial in the appropriate position in the head-space sampler.

11.2.12 Press the "Vial Parameter" key on the H-P 7964 head-space sampler, and enter the starting and stopping vial positions.

11.2.13 Press the "START" button on the H-P 7694 head-space sampler.

11.2.14 The head-space sampler will heat the sample for 60 min at 150°C and then automatically inject the head-space gas and start the gas chromatograph and integrator.

11.2.15 The final report will appear on the H-P 6890 integrator or the data system when the GC is finished. This report will give the micrograms of AA.

11.2.16 To determine the concentration in ppm of AA in the polymer sample, divide the micrograms of AA (reported in 11.2.15) by the sample weight in the vial (recorded in 11.2.9 as grams of polymer).

12. Calculation

12.1 The AA response factor is calculated as described in 9.11 and 9.12. The ppm of AA can be calculated manually by multiplying the response factor and the area of the AA peak, and then dividing this number by the sample weight in the vial (in grams).

13. Report

13.1 Report the ppm of AA to two decimal places.

14. Precision and Bias

14.1 The following was taken from work completed by the International Society of Beverage Technologists (ISBT) sub-committee concerning standardization of method to determine residual AA in PET.

14.2 The number of laboratories, materials, and determinations in this study meets the minimum requirements for determining precision in accordance with Practice E 691. A complete report is on file at ASTM Headquarters.⁴

⁴ Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:F02-1015.

14.3 This round robin was conducted by having one laboratory mold PET preforms on a 48-cavity injection molding machine and selecting 6 of those cavities as the sample set. Even though these preforms all came from one PET sample (material), each cavity has its own unique AA value, and thus, were treated as six different materials. Also, two different types of precision and bias were calculated, one based on each laboratory using their own calibration standard solution and another when each laboratory calibrated with a "common" calibration standard.

| | Practice E 691 Study | Minimum |
|-----------------|----------------------|---------|
| Laboratories: | 6 | 6 |
| Materials: | 6 | 4 |
| Determinations: | 3 | 2 |

14.4 *Precision and Bias With Each Laboratory Using Their Own Calibration Standard*—Precision, characterized by repeatability, Sr and r , and reproducibility, SR and R , has been determined for the materials to be as follows:

| Materials | Average | Sr | SR | r | R |
|------------|---------|--------|--------|--------|--------|
| Material A | 5.21 | 0.1812 | 0.6403 | 0.5074 | 1.7928 |
| Material B | 6.25 | 0.4060 | 0.7464 | 1.1368 | 2.0899 |
| Material C | 6.37 | 0.2880 | 0.6713 | 0.8066 | 1.8796 |
| Material D | 7.21 | 0.3285 | 0.7743 | 0.9198 | 2.1680 |
| Material E | 7.01 | 0.4217 | 0.8350 | 1.1808 | 2.3380 |
| Material F | 5.88 | 0.3930 | 0.7168 | 1.1003 | 2.0071 |

14.4.1 Since the materials used in this study are all from one specific type of material (PET), but have different AA levels because they are from different cavities, it makes more sense to have one set of precision values rather than one for each cavity. This will be derived by squaring each Sr and SR , averaging each of Sr^2 and SR^2 across materials and taking the square root.

| Sr | SR | r | R |
|--------|--------|--------|--------|
| 0.3466 | 0.7335 | 0.9705 | 2.0538 |

14.4.1.1 *Standard Deviation (Sr)*— Sr is the square root of the average within laboratory variance.

14.4.1.2 *Standard Deviation (SR)*— SR is the square root of the sum of the within laboratory variance and between laboratory variance of the laboratory means.

14.4.1.3 *Repeatability*— r is the interval representing the largest expected difference between two test results for the same material, obtained by the same operator using the same equipment on the same day in the same laboratory. A difference larger than r indicates more variation is present than expected.

14.4.1.4 *Reproducibility*— R is the interval representing the largest expected difference between two test results for the same material, obtained by different operators using different equipment in different laboratories, not necessarily on the same day. A difference larger than R indicates more variation is present than expected.

14.5 *Precision and Bias When Each Laboratory Uses a Common Calibration Standard*—Precision, characterized by repeatability, Sr and r , and reproducibility, SR and R , has been determined for the materials to be as follows:

| Materials | Average | <i>S_r</i> | <i>S_R</i> | <i>r</i> | <i>R</i> | <i>S_r</i> | <i>S_R</i> | <i>r</i> | <i>R</i> |
|------------|---------|----------------------|----------------------|----------|----------|----------------------|----------------------|----------|----------|
| Material A | 5.42 | 0.1849 | 0.4128 | 0.5178 | 1.1596 | 0.3376 | 0.5518 | 0.9453 | 1.5450 |
| Material B | 6.47 | 0.4123 | 0.6438 | 1.1545 | 1.8026 | | | | |
| Material C | 6.59 | 0.2703 | 0.5020 | 0.7567 | 1.4057 | | | | |
| Material D | 7.45 | 0.3113 | 0.6333 | 0.8716 | 1.7732 | | | | |
| Material E | 7.26 | 0.4014 | 0.5747 | 1.1240 | 1.6090 | | | | |
| Material F | 6.10 | 0.3854 | 0.5085 | 1.0792 | 1.4237 | | | | |

14.5.1 Since the materials used in this study are all from one specific type of material (PET), but have different AA levels because they are from different cavities, it makes more sense to have one set of precision values rather than one for each cavity. This will be derived by squaring each *S_r* and *S_R*, averaging each of *S_r²* and *S_R²* across materials and taking the square root.

14.6 *Bias*—There are no recognized polymer standards by which to estimate bias of this test method. Testing a known liquid standard with all laboratories using common calibration did not show any laboratory bias between laboratories or between the average of all laboratories and the known value.

15. Keywords

15.1 AA test; acetaldehyde; carbonated soft drink; ground parison AA; PET bottles; 24 hours headspace; water

APPENDIXES

(Nonmandatory Information)

X1. HEWLETT-PACKARD 6890 SERIES GC CONDITIONS

TABLE X1.1 Hewlett-Packard 6890 Series GC Conditions

| | |
|------------------------|--------------------|
| Temp 1 Isothermal | 90°C |
| Time 1 | 8.00 min |
| Injector Temperature | 250°C |
| Detector Temperature | 250°C |
| Head Pressure | 10 psi |
| Column-Flow | 12.2 mL/min Helium |
| Velocity | 85 cm/s |
| Split Ratio | 2.0 |
| Detector Air Flow | 300 mL/min |
| Detector Hydrogen Flow | 30 mL/min |
| Detector Makeup Flow | 20 mL/min helium |

X2. HEWLETT-PACKARD 7694 HEAD-SPACE SAMPLER CONDITIONS

TABLE X2.1 Hewlett-Packard 7694 Head-Space Sampler Conditions

| | |
|--------------------|----------|
| Oven Temp | 150°C |
| Loop Temp | 160°C |
| Transfer Line Temp | 170°C |
| Carrier Pressure | 11.5 psi |
| Vial Pressure | 10.5 psi |
| Vial Eq. Time | 60 min |
| Pressurize Time | 0.2 min |
| Loop Fill Time | 0.2 min |
| Loop Eq. Time | 0.1 min |
| Inject Time | 0.2 min |
| GC Cycle Time | 9 min |

X3. HEWLETT-PACKARD 6890 SERIES INTEGRATOR METHOD FILE

* LIST: METH @

RUN PARAMETERS

ZERO = 0
ATT 2^ = 0
CHT SP = 0.5
AR REJ = 200
THRSH = -2
PK WD = 0.04

TIMETABLE EVENTS

EMPTY

CALIBRATION

ESTD

REF % RTW: 5.000 NON-REF % RTW: 5.000

LEVEL: 1 RECALIBRATIONS: 3

| | | | | |
|------|-------|----|------------|------------|
| CAL# | RT | LV | AMT | AMT/AREA |
| 1R | 2.545 | 1 | 1.5030E+00 | 1.4933E-04 |

CAL# NAME
1 ACETALDEHYDE

INTEGRATION PLOT TYPE FILTERED
Presentation plot NO

RUN DATA STORAGE

Store signal data YES
Device M
Bunched or raw data RAW
Store processed peaks NO

CALIBRATION OPTIONS

RF of uncalibrated peaks 0.0000E+00
Calibration fit P
Disable post-run RT update .. NO
SAMPLE AMT 1.0000E+00
MUL FACTOR 1.0000E-02

REPORT OPTIONS

Suppress local report NO
HEIGHT% report NO
Report uncalibrated peaks ... YES
Extended report YES

PRINT & POST-RUN LIST OPTIONS

Large font YES
Store post-run report NO
External post-run report NO
List run parameters NO
List timetable NO
List calibration table NO
List remote method NO
Form-feed before report NO
Form-feed after report NO
Skip perforations in report .. NO
Skip perforations in plot ... NO
RANGE: C1,BUFFER 5!, 5!
INJECTOR 1 (not installed)
INJECTOR 2 (not installed)
TRAY (not installed)

FIG. X3.1 Hewlett Packard 6890 Series Integrator Method File

HP 6890 Series Gas Chromatograph 14 Feb 96 10:30

OVEN OVEN TEMPERATURE PROGRAM

| | | | | |
|--------------------|-----------|--------|------------|------------|
| Temp | 90 deg C | # Rate | Final temp | Final time |
| Initial time | 8.00 min | ----- | ----- | ----- |
| Maximum temp | 450 deg C | 1 | 0.00 | (off) |
| Equib time | 2.00 min | | | |

CRYO (not installed)

FRONT INLET (Split/Splitless) BACK INLET (Split/Splitless)

| | | | |
|-------------------|-------------|-------------------|-----------|
| Mode | Split | Mode | Split |
| Temp | 250 deg C | Temp | 250 deg C |
| Pressure | 10.0 psi | Pressure | 10.0 psi |
| Split ratio | 50.0 | Split ratio | 2.0 |
| Split flow | 87.7 mL/min | Split flow | 25 mL/min |
| Gas saver | Off | Gas saver | Off |
| Gas type | He | Gas type | He |

COLUMN 1

| | | | |
|------------------------|-------------------|------------------------|-------------------|
| Length | 30.0 m | Length | 30.0 m |
| Diameter | 320 u | Diameter | 530 u |
| Film thickness | 0.00 u | Film thickness | 5.00 u |
| Inlet | Front | Inlet | Back |
| Detector | Front | Detector | Back |
| Vacuum correct | Off | Vacuum correct | Off |
| Pressure correct | Off | Pressure correct | Off |
| Pressure | 10.0 psi | Pressure | 10.0 psi |
| Flow | 1.8 mL/min | Flow | 12.2 mL/min |
| Velocity | 32 cm/sec | Velocity | 85 cm/sec |
| Mode | Constant pressure | Mode | Constant pressure |

FRONT DET (Flame Ionization)

| | | | |
|--------------------|-----------------|--------------------|-----------------|
| Temp | 250 deg C | Temp | 250 deg C |
| H2 flow | Off | H2 flow | 30.0 mL/min |
| Air flow | Off | Air flow | 300 mL/min |
| Mode | Constant makeup | Mode | Constant makeup |
| Makeup flow | Off | Makeup flow | 20 mL/min |
| Makeup gas | He | Makeup gas | He |
| Flame | Off | Flame | On |
| Lit offset | 2.0 pA | Lit offset | 2.0 pA |
| Electrometer | On | Electrometer | On |

SIGNAL 1

| | | | |
|-------------|------|-------------|------|
| Type: | Back | Type: | Back |
| Zero | 0.0 | Zero | 0.0 |
| Range | 0 | Range | 0 |
| Attn | 0 | Attn | 0 |

COLUMN COMP 1 (no data)

COLUMN COMP 2 (no data)

FIG. X3.1 Hewlett Packard 6890 Series Integrator Method File (continued)

AUX 1 **VALVES**

| | | | | |
|------------|---------------|---------------|---------------|---------------|
| Temp | Not installed | Valve 1 | Not installed | |
| # Rate | Final temp | Final time | Valve 2 | Not installed |
| ----- | --- | ----- | Valve 3 | Not installed |
| | | | Valve 4 | Not installed |

AUX 2

| | | | | |
|------------|---------------|---------------|---------------|---------------|
| Temp | Not installed | Valve 5 | Not installed | |
| # Rate | Final temp | Final time | Valve 6 | Not installed |
| ----- | --- | ----- | Valve 7 | Not installed |
| | | | Valve 8 | Not installed |

AUX 3

| | |
|--------------------|----------|
| Pressure | Off |
| Initial time | 0.00 min |

AUX 3 PRESSURE PROGRAM

| | | |
|--------|------------|------------|
| # Rate | Final pres | Final time |
| ----- | --- | ----- |
| 1 | 0.00 | (off) |

AUX 4

| | |
|--------------------|----------|
| Pressure | Off |
| Initial time | 0.00 min |

AUX 4 PRESSURE PROGRAM

| | | |
|--------|------------|------------|
| # Rate | Final pres | Final time |
| ----- | --- | ----- |
| 1 | 0.00 | (off) |

AUX 5

| | |
|--------------------|----------|
| Pressure | Off |
| Initial time | 0.00 min |

AUX 5 PRESSURE PROGRAM

| | | |
|--------|------------|------------|
| # Rate | Final pres | Final time |
| ----- | --- | ----- |
| 1 | 0.00 | (off) |

RUN TABLE


No entries

FIG. X3.1 Hewlett Packard 6890 Series Integrator Method File (continued)

X4. CHROMATOGRAM OF A TYPICAL SAMPLE

* RUN # 238 JUN 5, 1996 08:36:16

START

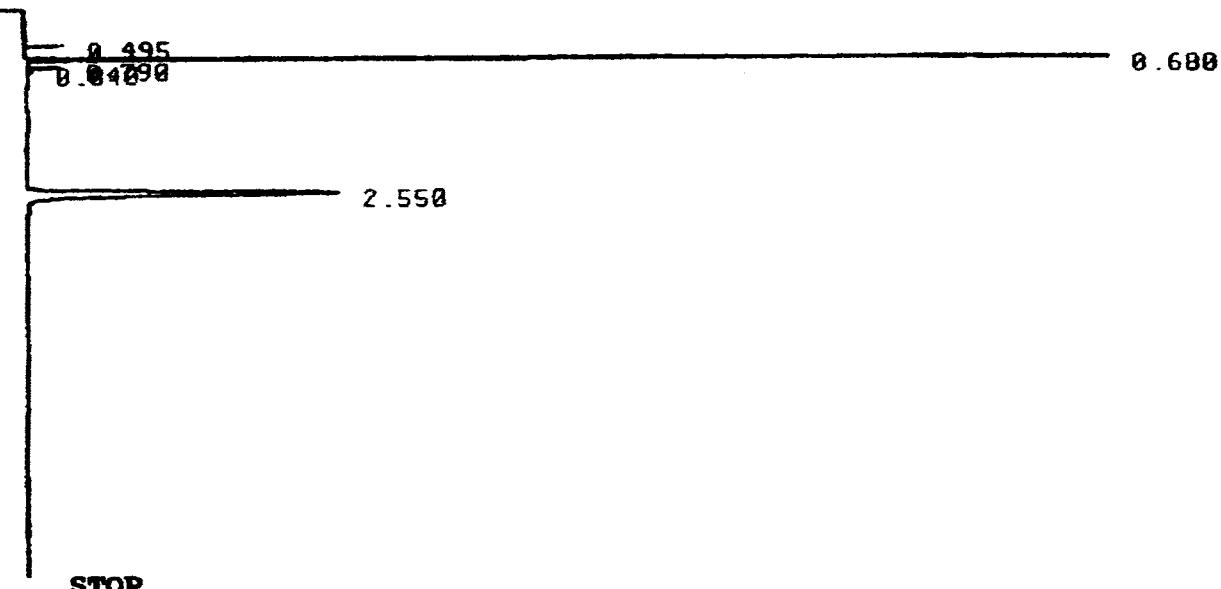

Closing signal file M: SIGNAL .RAW

RUN# 238 JUN 5, 1996 08:36:16

METHOD NAME: M:M18AAF.MET

SIGNAL FILE: M: SIGNAL.RAW

ESTD%-AREA

| RT | TYPE | AREA | WIDTH | CAL% | AMOUNT | NAME |
|-------|------|-------|-------|------|--------|--------------|
| .680 | PB | 27112 | .009 | | .000 | |
| 2.550 | PB | 9753 | .070 | 1R | 1.456 | ACETALDEHYDE |

TOTAL AREA= 36865

MUL FACTOR=1.0000E-02

SAMPLE AMT=1.0000E+00

FIG. X4.1 Chromatogram of a Typical Sample

X5. PREPARATION OF ACETALDEHYDE CALIBRATION STANDARDS

X5.1 Introduction

X5.1.1 The acetaldehyde (AA) calibration standards are used for calibrating gas chromatographs in the determination of AA present in PET preforms which are used in the food and beverage industry.

X5.2 Materials

X5.2.1 The materials for AA calibration standards are as follows:

X5.2.1.1 Distilled water.

X5.2.1.2 1-L Class A volumetric flask.

- X5.2.1.3 Sylon CT.
- X5.2.1.4 Acetaldehyde.
- X5.2.1.5 Syringe (1 mL).
- X5.2.1.6 Amber caps (4 mL).
- X5.2.1.7 Hole caps and TFE-fluorocarbon-faced septa.
- X5.2.1.8 Glass tray.
- X5.2.1.9 Balance (capable of 1-mg readings).
- X5.2.1.10 Refrigerator, set at 4°C.

X5.3 Setup

X5.3.1 Use distilled water that is stored in a container other than PET (that is, high-density polyethylene or polyvinyl chloride bottles)

X5.3.2 If this is the first time a 1-L Class A volumetric flask is being used or the flask has been used for something other than AA preparation, then proceed to **X5.3.3**. If the flask has been used previously for AA solution preparation, then proceed to **X5.3.4**.

X5.3.3 The flask must be deactivated which is done with Sylon CT, or equivalent.

X5.3.4 Using the distilled water described in **X5.3.1**, fill the deactivated or previously used 1-L flask to the fill line using the meniscus.

X5.3.5 Place the flask in a refrigerator and allow it to cool and equilibrate to ~4°C.

X5.3.6 The following items should also be stored in the refrigerator at ~4°C including the acetaldehyde, a 1-mL syringe, a box of unopened 4-mL amber vials, and a glass tray.

X5.3.7 Prepare the caps by placing the TFE-fluorocarbon-faced septa in the aluminum “hole-in-cap” lids. Make sure that the TFE-fluorocarbon facing is on the inside so that it is between the rubber septum and the glass vial. Please note that caps do not have to be refrigerated.

X5.4 Procedure

X5.4.1 Remove the AA, syringe, and 1-L flask and place them beside the balance.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).

X5.4.2 Fill the syringe with AA, handling the syringe by the top, taking care not to touch the body of the syringe, thereby causing it to heat up. Place the syringe on the balance and tare it.

X5.4.3 Remove the glass stopper from the 1-L flask, then insert the tip of the syringe into the water and discharge the AA. Remove the syringe and touch the inside sidewall of the flask to remove any drops. Recap the flask and weight the empty syringe immediately and record the weight loss.

X5.4.4 Invert the flask and shake at least ten times to ensure proper mixing of the AA.

X5.4.5 Remove the glass tray and the box of vials from the refrigerator. Place no more than 10 vials in the tray. The purpose of the tray is to catch overfill material.

X5.4.6 Using the 1-L AA solution in the flask, remove the stopper and fill the vials to above the brim, then re-stopper the flask.

X5.4.7 Cap all of the vials with the caps prepared in **X5.3.7**. It is important to complete **X5.4.6** and **X5.4.7** as quickly as possible to prevent AA loss.

X5.4.8 Repeat **X5.4.6** and **X5.4.7** until the desired amount of vials have been filled, never filling more than 10 at a time.

X5.4.9 For every five vials prepared, prepare one control vial of distilled water. This can be done at room temperature. This should be done after **X5.5.1** and **X5.5.3** have been completed as to prevent mislabeling.

X5.4.10 Check all vials to ensure they have no air bubbles (discard vials with air bubbles).

X5.5 Labeling

X5.5.1 Prepare labels containing the concentration listed as XXX milligrams of AA/litre of solution using the value obtained in **X5.4.3** as well as the current date.

X5.5.2 Prepare labels for the control vials saying distilled water.

X5.5.3 Place labels on the appropriate vials.